

Step 1: Receive

- Receive and Remove the product from the shipping sleeve
- Gently pull the tab from the box
- DO NOT THROW BOX AWAY - this is your return box!

Step 2: Use Preparation





- Remove Instructions and itemized list of contents from the box lid (Place documents in a safe place for future reference)
- Open large plastic bag holding the containers. (NOTE: the large plastic bag WILL be used in repackaging for return shipment)
- Take out the containers and place them in a safe space

Step 3: Use

- Twist lock to the unlock position and press down on the tab to open container
- Fill container with approved materials

Step 4: Return Preparation

- Once the containers are full, close the lid on the container and twist lock into the lock position
- Remove the return materials (plastic bag, tie wraps, tape and return label) from the inside lid of the return box
- Place the container inside the plastic return bag
- Gather the plastic and seal with tie wraps
- Place filled sealed containers inside the return box
- Fill out the itemized list of contents and place the document inside the return box
- Gather plastic of large bag and seal with tie wraps
- Close and seal the return box with provided packaging tape
- Return via UPS

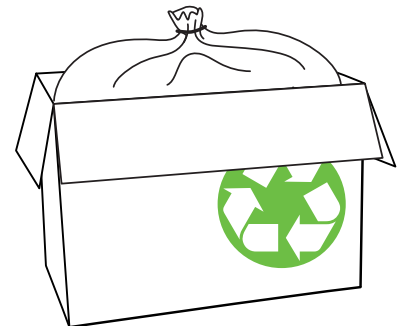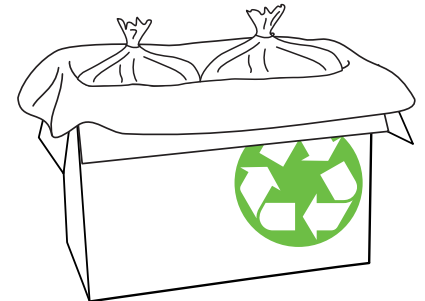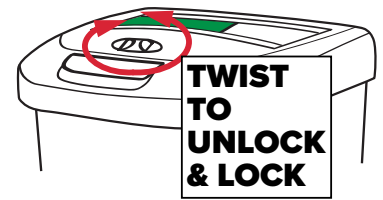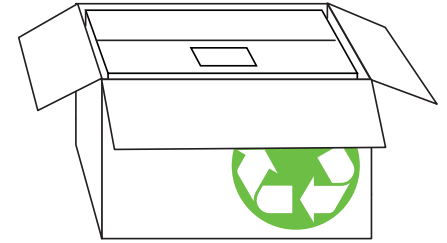

Make sure to reorder when supplies get low!

Questions?

Call 800-876-8264 or Email nxtmed@medsourcelabs.com

NxtMed™ is a MedSource Labs Company

Do's


- Drain any liquid from single use medical device
- Place all used, expired opened or unopened single use medical devices inside

Don'ts

- Glass Vials
- No Needles, Sharps or Syringes
- No Liquids
- No Mercury containing devices

Examples of Approved Materials:

Nasopharyngeals
Single use laryngoscopes
Single use laryngoscope blade
Single use laryngoscope handle
Endotracheal tubes
Nasal cannula
Laryngeal airway mask
Non-rebreathers
Oxygen tubing

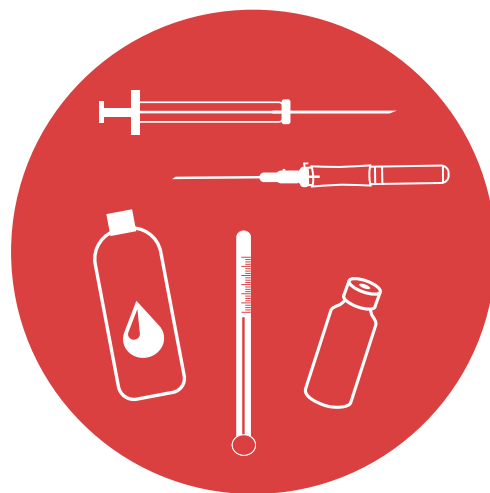

Questions?

Call 800-876-8264 or Email nxtmed@medsourcelabs.com

NxtMed™ is a MedSource Labs Company